


MI007 60 MHz Oscilloscope Probe User's Guide



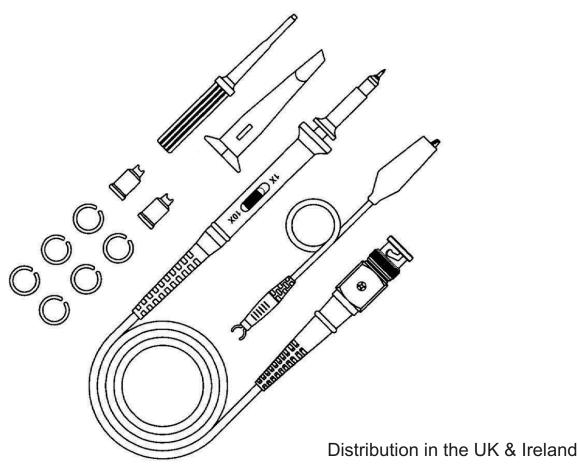

Lambda Photometrics Limited


Lambda House Batford Mill Harpenden Herts AL5 5BZ United Kingdom

E: info@lambdaphoto.co.uk W: www.lambdaphoto.co.uk


T: +44 (0)1582 764334 F: +44 (0)1582 712084

Frequency Compensation

Before taking any measurements using a probe, first check the compensation of the probe and adjust it to match the channel inputs. Most oscilloscopes have a square wave reference signal available at a terminal on the front panel used to compensate the probe. Connect the probe to this terminal or another 2 V pk-pk, 1 kHz square wave source. Set the probe to 10X position. Adjust trimmer until seeing flat-top square wave on the display.

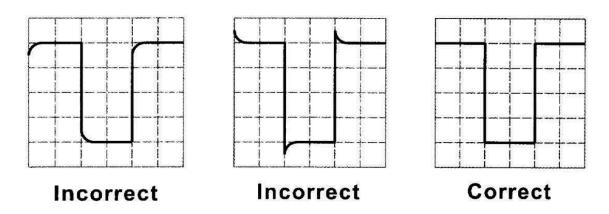


Voltage vs Frequency Rating Curve

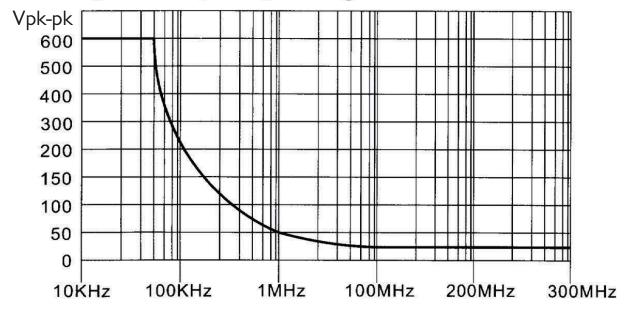


Review this user manual carefully to avoid injury and prevent damage to this product or any products connected to it. To avoid potential hazards, use this product only as specified.

Accessories and Features

MI007 is provided with several accessories designed to make probing and measurement simpler. Please take a moment to familiarize yourself with these accessories and their uses.

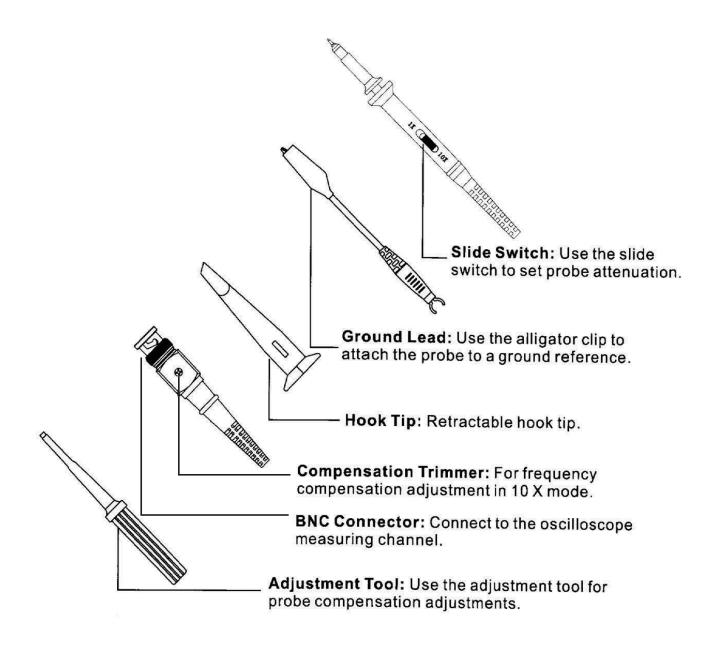

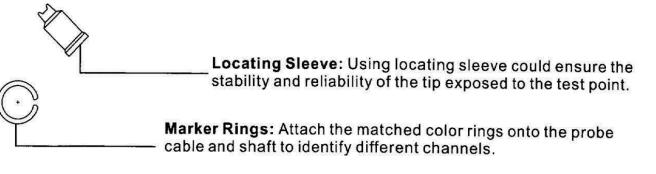

Probe Characteristics			
Attenuation Ratio	1X	10X	
Bandwidth	15 MHz	60 MHz	
Rise Time	23.3 ns	5.8 ns	
Input Resistance	1 MΩ ± 2%	10 MΩ ± 2%	
Input Capacitance	70pF~120pF	14pF~18pF	
Maximum Working Voltage (CAT I)	200 V pk-pk	600 V pk-pk	
Compensation Range		15 - 45pF	
Operation Environment	0 - 50°C, 0 - 80%RH		
Storage Environment	-20 - 60°C, 0 - 90%RH		
Size	110 ±2cm		
Weight	About 55g		

Accessory Kit			
	MI007	TA208	
Description	1PC	2PC	
Retractable Hook Tip	1	2	
Adjustment Tool	1		
Locating Sleeve	2		
Marker Rings	6		
Ground Lead	1	2	