

Distribution in the UK & Ireland



Lambda Photometrics Limited

Lambda House Batford Mill
Harpenden Herts AL5 5BZ
United Kingdom

E: info@lambdaphoto.co.uk

W: www.lambdaphoto.co.uk

T: +44 (0)1582 764334

F: +44 (0)1582 712084

SCHOTT
glass made of ideas

KL 300 LED

User Manual




Contents



1.	Important information.....	3
2.	Operation.....	5
2.1	Assembly.....	5
2.2	Light guide connection.....	5
2.3	Power connection.....	6
2.4	Start-up procedure.....	6
2.5	Light intensity setting.....	6
3.	Maintenance.....	7
4.	Troubleshooting.....	7
5.	Accessories.....	7
6.	Technical data.....	8

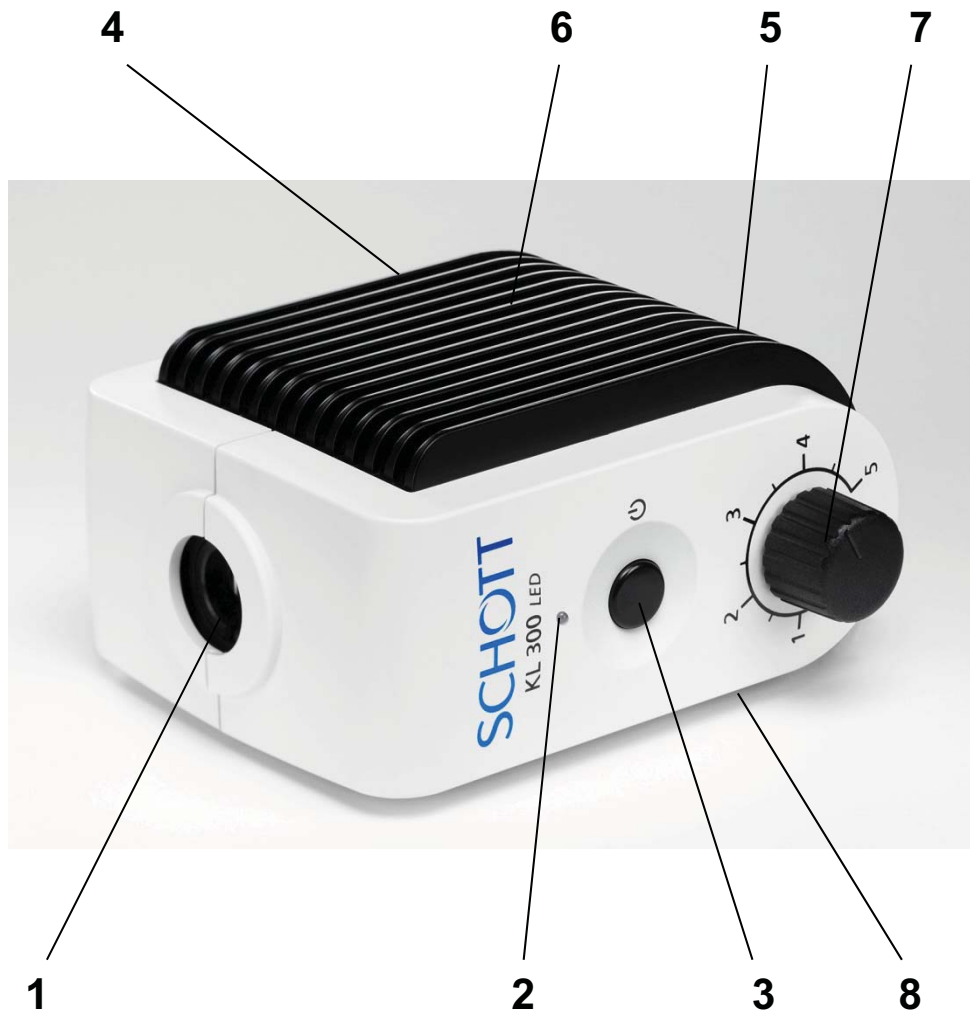

Instrument overview



(1)	Light guide socket	2.2
(2)	Indicator light	2.4
(3)	On/off switch	2.4
(4)	Mains connection socket	2.3
(5)	Attachment adapter socket (base of instrument)	2.1
(6)	Heat sink	
(7)	Electronic light intensity setting	2.5
(8)	Model plate (base of instrument)	

1. Important information

Symbols used

Symbol	Meaning
	Warning of danger (caution, obey documentation)
	LED-radiation (caution, do not look directly into the beam!)

Intended use

The KL 300 LED cold light source is intended for industrial and laboratory applications.

Cold light sources are used for the intensive illumination of all types of objects. High-intensity visible light is guided to the object using flexible or self-supporting, movable light guides.

In accordance with the EN 62471:2008 standard the KL 300 LED is a product of Risk Class 2.

The KL 300 LED fiber optic light source conforms to the following European directives:

2014/35/EU (Low Voltage Directive)

2014/30/EU (EMC Directive)

2011/65/EU (RoHS)

The technical documentation and full compliance with the standards listed below proves the conformity with the essential requirements of the following EC Directives:

EN 61326-1:2013

EN 61010-1:2010

EN 50581:2012



Safety information:

Please read and obey these instructions carefully. The instrument's safety cannot be guaranteed if they are not obeyed.

Do not look directly into the open light guide socket or the light guide exit when the light source is switched on (danger of ophthalmic injury)!

The KL 300 LED emits high-intensity visible light. Because light-absorbing materials have the physical property of converting incident light into heat, damage can arise to heat-sensitive or flammable light-absorbing materials. To avoid such thermal damage and the potential danger of fire or burns, please obey the following instructions:

KL 300 LED – Operating instructions


- Never cover up the light guide socket or light guide exit (danger of fire)!
- Never cover up the open light guide socket or light guide exit with your hands or other parts of the body (danger of burns)!
- When illuminating heat-sensitive or flammable light-absorbing objects (e.g. in microscopy), special care must be taken to ensure that an appropriate suitable distance between light guide and object, and a suitable lamp brightness level are selected so that no thermal damage occurs.
- When the light source is switched on, all light guide exists not being used in the working procedure must always be a safe distance – at least 10 cm – away from heat-sensitive or flammable light-absorbing materials (prevention of possible danger of fire). Care must, therefore, be taken that each light guide exit is at the above-mentioned safe distance away from, for example, dark/colored textiles and dark/colored wooden or plastic surfaces.
- To avoid unnecessary stressing of biological tissue by illuminating with visible light, reduce the brightness and duration of illumination to the absolute minimum required level.

Please make sure that your KL 300 LED cold light source is operated at the voltage stated on the model plate (8).

- The light source has been developed for operation in dry rooms only! (see Point 6 “Technical Data”)!
- The instrument must not be used in explosive areas.
- Safe disconnection from the power supply occurs only by pulling out the mains plug.
- The instrument may neither be opened nor dismantled. Technical modifications are forbidden. Repairs must only be carried out by the manufacturer or by its authorized customer service agency.
- Please ensure that every user of the system has quick access to these operating instructions.
- The manufacturer is not liable for damage caused by failure to obey these instructions.

2. Operation

2.1 Assembly

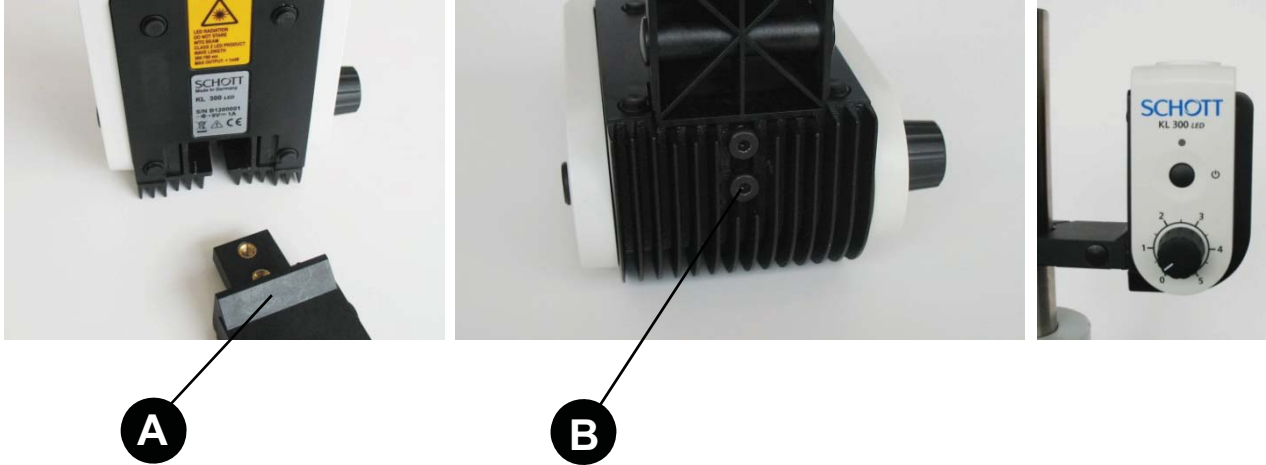

KL 300 LED is designed for assembly directly on all conventional microscope objectives or swivel arm stands. Suitable adapters are either enclosed with the light source or are available from the manufacturer (see Point 5 “KL 300 LED accessories”).

First insert the appropriate side of the attachment adapter (A) into the intended socket (5) on the base of the light source until stop. Then insert both fixing screws (M5) from below through the groove (B) and tighten using a 3-mm Allen key.

The light source can now be clamped to the microscope objective or swivel arm stand with the attachment adapter. If necessary, the microscope or the microscope carrier must be taken off and re-assembled afterwards.

Alternatively, when using flexible light guides, the KL 300 LED can be laid flat on the work surface without an attachment adapter.

2.2 Light guide connection



The light guide is inserted into the light guide socket as far as the stop (1). To ensure a tight fit and optimum illumination the groove must click into the retaining slot.

To remove, simply pull the light guide out of the light guide socket (1).

Please note: When inserting light guides with a locating pin, care must be taken to ensure that the pin fits into one of the two guide slots.

KL 300 LED – Operating instructions

2.3 Power connection

Insert the hollow plug of the supplied power cord into the plug-in socket (4) of the light source.

Please take care to ensure that you only operate your KL 300 LED light source with the power cord provided.

The plug connection of the power supply is interchangeable for the EU, UK, US or AU. This is connected to the mains supply (100-240 V AC, 50-60 Hz).



2.4 Start-up procedure



Switch on/off the KL 300 LED by pressing the switch (3).

When the instrument is switched on the blue control light (2) is lit.

Please disconnect power by pulling out the power plug.

2.5 Light intensity setting


The brightness can be adjusted continuously by turning the light intensity setting knob (7).

Five-step intensity control is possible, from 0 – 5.

The highest brightness is reached at the end stop at position 5.

When the brightness control is set at 0 there is no more brightness, i.e. the lamp is off.

Attention: Please note that when the brightness control is set at 0 the instrument is not switched off. When the instrument is switched on the blue control light (2) is lit. To switch off the KL 300 LED press the on/off switch (3) once (see point 2.4 “Start-up procedure”). Please ensure safe power disconnection by pulling out the power plug!

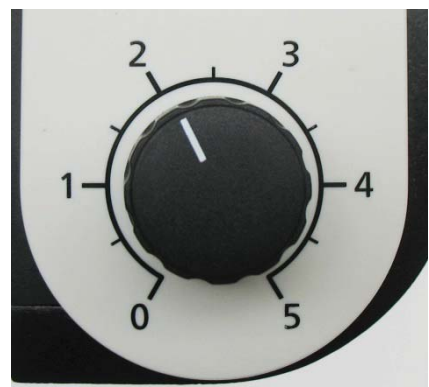

3. Maintenance

KL 300 LED – Operating instructions

Your KL 300 LED is maintenance-free.

The light source should not be disinfected for use in medical applications.

To clean the outside of the instrument please use a soft dry cloth or commercially available plastic cleaning cloths.

4. Troubleshooting

Should you be unable to rectify the faults by the measures listed below, please contact your specialist dealer or the nearest SCHOTT agency. More extensive repairs must be carried out by an authorized after sales service.

Fault	Possible cause	Remedial action
Lamp out	Instrument not switched on	Switch instrument on
	Plug not in socket	Plug in socket
	No mains electricity voltage	Check mains voltage
Light intensity dropping	Electronics overheated	Switch off instrument. Ensure adequate cooling, switch on again after prolonged cooling time.

5. KL 300 LED accessories

A wide range of accessories is available for your KL 300 LED. Please see our separate catalogue for further details (contact address for additional requirements can be found on page 10).

Proper functioning, safety and optimum luminous efficiency can only be guaranteed with SCHOTT light guides and accessories.

Self-supporting and flexible light guides are available in various lengths and diameters, as well as spot illuminations.

Optical filters can be used as screw-in or clip-on filters in conjunction with a focusing attachment (accessory) in front of the light guide exit.

Details on the focusing attachment and available standard filter types can be found in our catalogue.

Adapters for attaching the KL 300 LED to microscope objectives and swivel arm stands are available, either with this light source or they can be ordered separately. Please see our catalogue for further details on each type.

The light source can also be used as a “stand-alone” instrument if the light source is not mounted on an objective or a swivel arm. When using flexible light guides no accessories are required (see

KL 300 LED – Operating instructions

Point 2.1 “Assembly”). A base with a corresponding fixing device is available for use with self-supporting light guides. Please also refer to our catalogue for more information.

6. Technical data for KL 300 LED

Properties		Values
General information		
Type description		KL 300 LED
Dimensions (W x D x H)	mm	approx. 107 x 114 x 61
Weight	kg	approx. 0.35
Cooling		Convection
Ambient temperature*	°C	+ 5 ... + 40
Relative air humidity*	%	at 31°C ambient temperature: 80% From 31°C to 40°C ambient temperature: decreasing linearly to 50%
Air pressure*	hPa	800 ... 1060
Transport and storage		
Temperature	°C	-20 ... +70
Rel. air humidity	%	10 ... 95 (non-condensing)
Air pressure	hPa	500 ... 1200
Contamination level		2
Electrical information		
Operating voltage, frequency		100 - 240 V ~ 50 - 60 Hz
Rated current device		1 A
Nominal voltage device		9 V
Power consumption, max.	VA	max. 5
Protection class		II
Overvoltage category		II
Diode		High Power LED
LED nominal output	W	3
Average LED lifetime LED Level 5	h	50,000 (luminous flux reduced to 70%)

* Test conditions of DIN EN 61010-1 and UL61010-1 standards

KL 300 LED – Operating instructions

Lighting information	
Maximum effective light guide bundle diameter mm	6
Total light flux at light guide exit (SCHOTT light guide Ø 4.5 mm, typical values)	
Level 5 lm	80
Color temperature K	Approx. 5,600
Light exit angle ($2\alpha_{\text{eff}}$)	Approx. 53°
Conformity	CE
EMC emission class	(power supply CE, UL, PSE) B

We reserve the right to make changes in the design and supplied items within the scope of on-going technical improvements.



WEEE declaration

Your SCHOTT product was produced and developed with high quality materials and components. The symbol indicates that electrical and electronic devices must be separated from domestic waste and appropriately disposed of after useful life.

SCHOTT AG Lighting and Imaging has arranged a waste management system for recycling. Please use this system for removal and help to protect the environment we live in. Further information regarding our waste management system, please refer to

www.schott.com/lightingimaging/recycle

Distribution in the UK & Ireland



**Characterisation,
Measurement &
Analysis**

Lambda Photometrics Limited
Lambda House Batford Mill
Harpenden Herts AL5 5BZ
United Kingdom
E: info@lambdaphoto.co.uk
W: www.lambdaphoto.co.uk
T: +44 (0)1582 764334
F: +44 (0)1582 712084